

Environmental and economic impact of using increased fresh gas flow to reduce carbon dioxide absorbent consumption in the absence of inhalational anaesthetics

George Zhong^{1,*}, Ali Abbas², Joseph Jones², Sarah Kong¹ and Tim McCulloch^{3,4}

¹Department of Anaesthesia, Concord Repatriation General Hospital, Sydney, Australia, ²School of Chemical and Biomolecular Engineering, The University of Sydney, Sydney, Australia, ³Department of Anaesthesia, Royal Prince Alfred Hospital, Sydney, Australia and ⁴Sydney Medical School, The University of Sydney, Sydney, Australia

*Corresponding author. E-mail: drgzhong@gmail.com

Abstract

Background: Increasing fresh gas flow (FGF) to a circle breathing system reduces carbon dioxide (CO₂) absorbent consumption. We assessed the environmental and economic impacts of this trade-off between gas flow and absorbent consumption when no inhalational anaesthetic agent is used.

Methods: A test lung with fixed CO₂ inflow was ventilated via a circle breathing system of an anaesthetic machine (Dräger Primus or GE Aisys CS²) using an FGF of 1, 2, 4, or 6 L min⁻¹. We recorded the time to exhaustion of the CO₂ absorbent canister, defined as when inspired partial pressure of CO₂ exceeded 0.3 kPa. For each FGF, we calculated the economic costs and the environmental impact associated with the manufacture of the CO₂ absorbent canister and the supply of medical air and oxygen. Environmental impact was measured in 100 yr global-warming potential, analysed using a life cycle assessment 'cradle to grave' approach.

Results: Increasing FGF from 1 to 6 L min⁻¹ was associated with up to 93% reduction in the combined running cost with minimal net change to the 100 yr global-warming potential. Most of the reduction in cost occurred between 4 and 6 L min⁻¹. Removing the CO₂ absorbent from the circle system, and further increasing FGF to control CO₂ rebreathing, afforded minimal further economic benefit, but more than doubled the global-warming potential.

Conclusions: In the absence of inhalational anaesthetic agents, increasing FGF to 6 L min⁻¹ reduces running cost compared with lower FGFs, with minimal impact to the environment.

Keywords: anaesthesia machine; carbon dioxide absorbent; cost analysis; fresh gas flow; life cycle assessment; mechanical ventilation; total intravenous anaesthesia

Editor's key points

- The trade-off between the environmental and economic impacts of fresh gas flow and carbon dioxide (CO₂) absorbent consumption in anaesthetic machine breathing circuits was assessed in a simulation study.
- A test lung with fixed CO₂ inflow was ventilated via a circle breathing system of an anaesthetic machine at various fresh gas flows to determine time to exhaustion

of the CO₂ absorbent canister, with calculation of the economic costs and associated environmental impact.

- A significant cost saving may be derived by increasing fresh gas flows to reduce CO₂ absorbent consumption, with minimal adverse impact to the environment.
- High-flow anaesthesia is a viable cost-saving strategy when using a circle system for anaesthetic maintenance without inhalational anaesthetic agents in adults.

Received: 4 February 2020; Accepted: 10 July 2020

© 2020 British Journal of Anaesthesia. Published by Elsevier Ltd. All rights reserved.
For Permissions, please email: permissions@elsevier.com

Most modern anaesthetic machines use a circle breathing system, which facilitates use of low fresh gas flow (FGF) during maintenance of anaesthesia. Advantages of low FGF include reduced consumption of inhalational anaesthetic agents and conservation of expired heat and water vapour.¹ Disadvantages of low FGF include longer times for changes in fresh gas composition to affect inspired gas composition, accumulation of unwanted gases, and increased consumption of carbon dioxide (CO₂) absorbent.² When a circle system is used with total i.v. anaesthesia and an efficient heat and moisture exchange (HME) filter, the advantages of low FGF may no longer apply. Furthermore, using high FGFs confers the advantage of reduced CO₂ absorbent consumption.

Given that medical oxygen (O₂) and air are relatively inexpensive for most major hospitals, we hypothesise that the reduction in CO₂ absorbent consumption at high FGF may outweigh the associated cost and environmental impact of increased gas (medical O₂ and air) consumption during total i.v. anaesthesia. We therefore performed a laboratory study examining the relationship between FGF and time to exhaustion of absorbent canisters using two different anaesthetic machines, together with cost and environmental analyses.

Methods

A simple lung model (Fig. 1) was constructed using a 1 L test lung (SelfTestLung™; Dräger, Notting Hill, Australia) with CO₂ insufflated through the sample port of an HME filter (Thermovent® HEPA; Smiths Medical, Minneapolis, MN, USA) attached to the test lung. A second HME filter was attached to the Y-connection of the breathing circle to provide a sample port for capnography. To mimic anatomical dead space, a length of extension tubing (internal volume 90 ml) was placed between the two HME filters. The model was ventilated via a standard circle system with 1.8 m corrugated tubing and a 2 L reservoir bag.

The anaesthetic machine was connected to hospital piped medical gases and set to deliver an O₂/air mixture with fresh gas O₂ concentration of 30%. Fresh gas flows of 1, 2, 4, and 6 L

min⁻¹ were studied. The lung model was ventilated with the anaesthetic machine ventilator set to volume-control mode, ventilatory frequency of 12 bpm, tidal volume of 500 ml, and inspiratory-to-expiratory ratio of 1:1.5. End-tidal CO₂ (ETCO₂) and inspired CO₂ (InspCO₂) partial pressures were monitored via the capnography module of the anaesthetic machine and recorded every 5 min. Three runs were performed at each FGF, and the entire study was repeated using two different anaesthetic machines: the Dräger Primus® (Dräger, Lübeck, Germany; hereafter DG for short) and GE Aisys CS²® (GE, Chicago, IL, USA; hereafter GE for short). The endpoint for the study was time to exhaustion of the CO₂ absorbent, defined as InspCO₂ >0.3 kPa for 15 min, which we consider to be a reasonable threshold for changing the absorbent in clinical practice.

CO₂ inflow was from a cylinder regulated by a ball rotameter, which was calibrated daily using a digital flowmeter (VT MOBILE; Fluke Biomedical, Cleveland, OH, USA) and adjusted to deliver a flow of ~250 ml min⁻¹. Throughout all runs at FGFs of 1, 2, and 4 L min⁻¹, ETCO₂ remained between 5.1 and 5.6 kPa. For the longer runs at FGF of 6 L min⁻¹, ETCO₂ remained between 5.1 and 6.4 kPa. As the capnography waveform and ETCO₂ values produced by our model were representative of those observed during ventilation of healthy patients in clinical practice, we believe our model was a reasonable approximation for the purposes of this investigation.

The CO₂ absorbent was refreshed before each run. With the DG machine, a pre-packaged canister was used (Infinity ID CLIC™ Absorber; Dräger, Lübeck, Germany). The total weight of the canister was 1052 (10) g, with the empty plastic container weighing 112 (5) g. With the GE machine, a reusable canister was manually filled with 775 (5) g of absorbent pellets (Medisorb™ CO₂ Absorbent; CareFusion, San Diego, CA, USA), weighed using an electronic scale.

Economic analysis was performed using acquisition costs for medical O₂ and CO₂ absorbent for the Sydney Local Health District. We estimated the cost of medical air, which is produced on-site by electric compressors (ZT18; Atlas Copco,

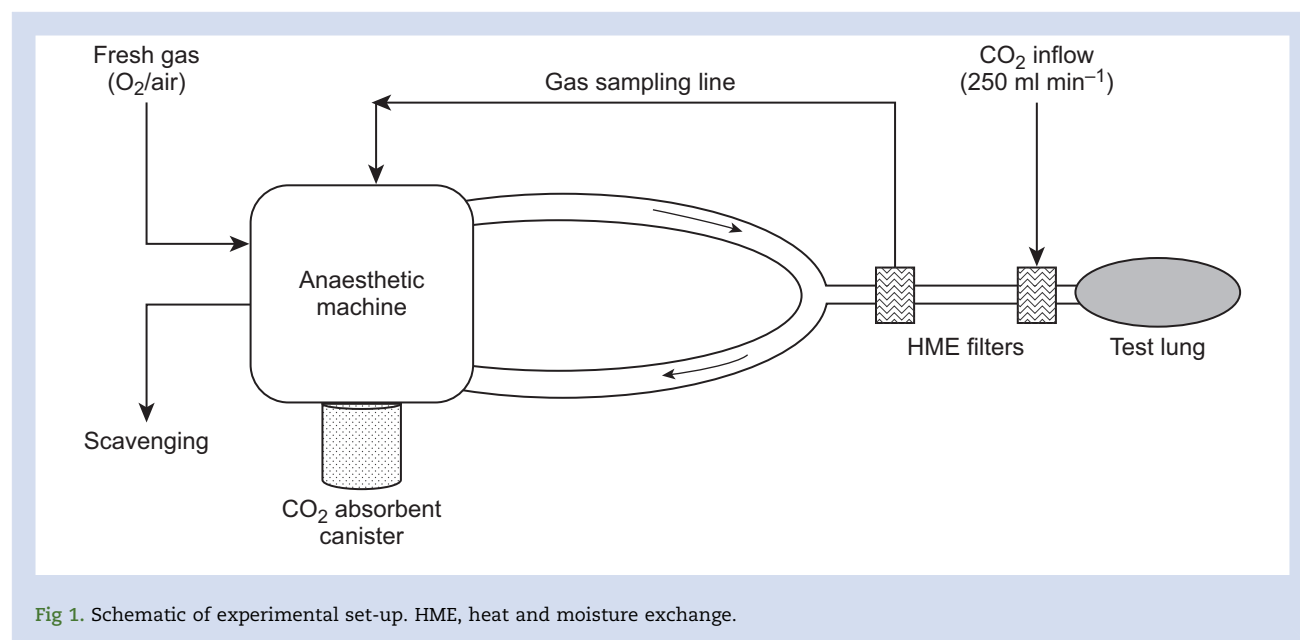


Fig 1. Schematic of experimental set-up. HME, heat and moisture exchange.

Table 1 Mean (standard deviation) time to exhaustion of CO₂ absorbent canisters, hourly cost, and environmental impact at various fresh gas flows for DG and GE anaesthetic machines. CO₂, carbon dioxide; DG, Dräger Primus; FGF, fresh gas flow; GE, GE Aisys CS²; GWP₁₀₀, 100 yr global-warming potential.

FGF (L min ⁻¹)	DG			GE		
	Time to exhaustion (h)	Cost (AU\$ h ⁻¹)	GWP ₁₀₀ (kg CO ₂ equivalent h ⁻¹)	Time to exhaustion (h)	Cost (AU\$ h ⁻¹)	GWP ₁₀₀ (kg CO ₂ equivalent h ⁻¹)
1	10.3 [0.3]	1.46	0.13	8.2 [0.4]	1.60	0.14
2	13.1 [0.6]	1.16	0.13	11.2 [1.1]	1.17	0.13
4	34.7 [1.2]	0.45	0.12	22.9 [1.3]	0.59	0.13
6	205.3 [29.7]	0.10	0.14	133 [22.2]	0.12	0.14
15	—	—	—	—	0.06	0.33
18	—	0.08	0.40	—	—	—

Antwerp, Belgium) and intercoolers (FD120; Atlas Copco, Milan, Italy), from their respective power ratings, the local cost of electricity, and the estimated equipment acquisition cost. Unless otherwise stated, all costs are reported in Australian dollars (AU\$).

Environmental analysis was carried out using a life cycle assessment (LCA) cradle-to-grave approach. Life cycle assessment is an analysis of the environmental impacts of all systems and material flows involved at any stage throughout the life of a product or service,³ and is a robust method for assessing the environmental performance of a product. The procedure for conducting an LCA is standardised in ISO 14040 and consists of four main stages: (i) definition of goal and scope, (ii) inventory analysis, (iii) impact assessment, and (iv) interpretation and evaluation.⁴ The impact category relevant to our current study is the 100 yr global-warming potential (GWP₁₀₀) given in kilograms of CO₂ equivalents. Our LCA accounts for the global-warming impact arising from the production, transport, and disposal of the CO₂ absorbent canister, medical O₂, and air. The canister is composed of absorbent material (a soda lime mixture of calcium hydroxide and sodium hydroxide) and the container itself is composed of polypropylene. The production of calcium hydroxide covers all equipment and total heating energy for production. The production of sodium hydroxide is assumed to be through electrolysis and covers brine production. The production of O₂ is assumed to be through an air separation plant and covers the electricity for the production process, cooling water, and waste heat and infrastructure. The production of air is assumed to include a compressor and electricity consumption. Transport of absorbent canisters is assumed to be by sea freight from their country of manufacture, and then by road to the institution. Disposal of the canisters and materials is assumed to be via landfill and is included in the scope of the study. Impact assessment for each of the production processes was performed with SimaPro (PRé Consultants BV, Amersfoort, Netherlands) using its inbuilt life cycle inventory database (ecoinvent 2.2).

All data processing was performed in Excel 365 (Microsoft Corporation, Redmond, WA, USA) and descriptive statistics were reported. Details of the economic and environmental analyses are described in the Supplementary material.

Results

The mean time to CO₂ absorbent canister exhaustion and the associated cost and environmental impact at various FGFs are shown in Table 1. The mean time to CO₂ absorbent canister exhaustion increases non-linearly with increasing FGFs for both DG and GE anaesthetic machines (Fig. 2a). A plot of FGF against the reciprocal of time to exhaustion, which represents the fraction of CO₂ absorbent canister being consumed per unit time, reveals a linear relationship (Fig. 2b). This linear relationship is consistent with previous studies.^{5,6} At FGF of 6 L min⁻¹, it took more than 5 days (GE) or 8 days (DG) for exhaustion of the absorbent.

Our estimated costs of medical O₂ and air were \$0.40 and \$0.028 (1000 L)⁻¹, respectively. The GWP₁₀₀ values associated with the production of 1 kg of medical O₂, air, CO₂ absorbent, and polypropylene were 0.70, 0.23, 0.73, and 3.53 kg CO₂ equivalents, respectively. Combining these results with the time to CO₂ absorbent exhaustion, we calculated the hourly running cost at each FGF (Fig. 3) and the hourly emissions in CO₂ equivalents (Fig. 4) associated with each FGF.

Increasing FGF is associated with a significant decrease in running cost with minimal net changes to environmental impact. Compared with FGF of 1 L min⁻¹, increasing FGF to 4 L min⁻¹ was associated with a 69% and 63% reduction in the running cost, and 6% and 5% reductions in the global-warming potential for DG and GE, respectively. Further increasing FGF to 6 L min⁻¹ was associated with 93% and 92% reductions in running costs and resulted in 9% increase and 0.2% decrease in global-warming potentials compared with FGF of 1 L min⁻¹ for DG and GE, respectively.

For comparison, we also calculated the costs and environmental impact associated with the hypothetical case, where CO₂ elimination from the circle system was entirely attributable to FGF. Removing the absorbent canister from the circle system, we found that FGFs of 18 and 15 L min⁻¹ were required to keep InspCO₂ below 0.3 kPa for DG and GE, respectively. This extreme case is associated with around 20-fold reduction in the running cost compared with FGF 1 L min⁻¹ with CO₂ absorbent present (from \$1.46 h⁻¹ and \$1.60 h⁻¹ to \$0.08 h⁻¹ and \$0.06 h⁻¹ for DG and GE, respectively). However, the global-warming potential was also more than doubled for both

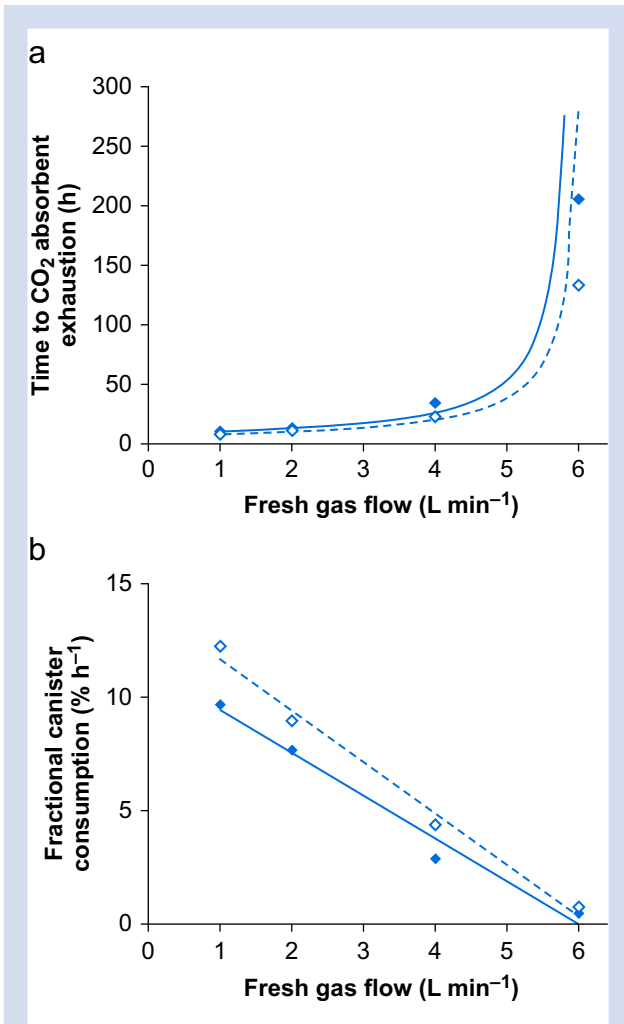


Fig 2. Impact of fresh gas flow on (a) time to exhaustion of CO₂ absorbent and on (b) CO₂ absorbent canister consumption rate for DG (◆) and GE (◇) anaesthetic machines. CO₂, carbon dioxide; DG, Dräger Primus; GE, GE Aisys CS²

cases (from 0.13 and 0.14 to 0.40 and 0.33 kg CO₂ equivalent h⁻¹, respectively).

To assess the generalisability of our economic analysis, we approached colleagues from tertiary hospitals across the UK and USA to obtain international cost data. Because of sensitivity of commercial information, we were only able to obtain approximate costs for medical O₂ and the Dräger CO₂ absorbent canister. To obtain a lower bound estimate of the reduction in running costs, we assumed an inspired O₂ fraction of 100% and used the highest cost for medical O₂ together with the lowest cost for the CO₂ absorbent canister that were obtained. We also extracted relevant cost data for Germany from a 2012 study.⁷ Compared with our Australian data, similar trends in running cost reduction were found for UK, USA, and Germany (see Supplementary material).

To assess the generalisability of our environmental analysis, we examined the effect of including absorbent canister transport via sea freight from the country of manufacture (Germany) into the bounds of the LCA, and considered

shipping to Australia, UK, and USA. We found this made little difference to the overall trend in CO₂ emission at various FGFs (see Supplementary material).

Discussion

We confirmed that the time to CO₂ absorbent exhaustion is significantly prolonged by increasing the FGF within the circle systems of both the DG and GE anaesthetic machines. These results are in line with previous *in vitro* studies of absorbent consumption.^{5,6,8} By combining the relationship between FGF and absorbent exhaustion time with local cost data, we have shown that there are potential cost savings when FGFs over 4 L min⁻¹ are used without inhalational anaesthetic agents. Our LCA found that the combination of increased FGF up to 6 L min⁻¹ with reduced absorbent consumption has little to no net impact on the global-warming potential.

Multiple mechanisms have been proposed to explain the reduction in absorbent consumption associated with increasing FGFs for circle systems.⁸ Higher FGF results in dilution of CO₂-containing gas within the expiratory limb during the expiratory phase, reduction in expired gas circulating to the inspiratory limb during the inspiratory phase, and increased clearance of CO₂ via the effluent gas during expiration and during the pause between end expiration and inspiration. All mechanisms ultimately lead to a reduction in exposure of the absorbent canister to CO₂, thereby prolonging the time to exhaustion. In addition to these circuit factors, it is also possible that at high FGFs, CO₂-containing expired gas can access parts of the canister that would not be reached at lower FGFs, resulting in more efficient absorption. Higher FGFs can also reduce moisture content within the canister, thereby reducing clumping and thus channelling of CO₂-containing expired gas through the canister, which indirectly prolongs exhaustion time.

A potential problem with higher FGF is drying of the inspired gases. Previous studies⁹ have estimated the lowest acceptable limit for absolute humidity of inhaled gas during brief (<2 h) anaesthetic procedures to be 20 mg L⁻¹ and for prolonged ventilation in intensive care to be 30 mg L⁻¹. However, modern HME filters are highly efficient at maintaining the inspired humidity well above the acceptable limit across a wide range of FGFs.¹⁰ Using a modern HME filter together with FGF of 6 L min⁻¹, it has been found that the absolute humidity within the airway was 29 mg L⁻¹ after 120 min of mechanical ventilation under general anaesthesia, far exceeding the acceptable minimum.¹¹ Similar results were found in another study¹² using FGF of 5 L min⁻¹. Thus, high FGFs up to 6 L min⁻¹ are safe in terms of gas humidity in adults when a modern HME filter is used.

Another concern regarding the use of high FGFs is the risk of desiccating the CO₂ absorbent, which can potentially lead to increased carbon monoxide production during a subsequent volatile anaesthetic procedure using the same canister. However, this concern is theoretical with modern CO₂ absorbents, which have much lower strong alkali content, and it has been shown that carbon monoxide production remains undetectable (<10 ppm), even when the absorbent is subjected to more exaggerated drying conditions compared with our study.¹³

Our study has several limitations. We only examined a single set of ventilation parameters. It is known that the ventilation pattern can affect the flow characteristics within the circle system, and thus influence the amount of CO₂ reaching the absorbent canister.⁵ For example, prolonging the

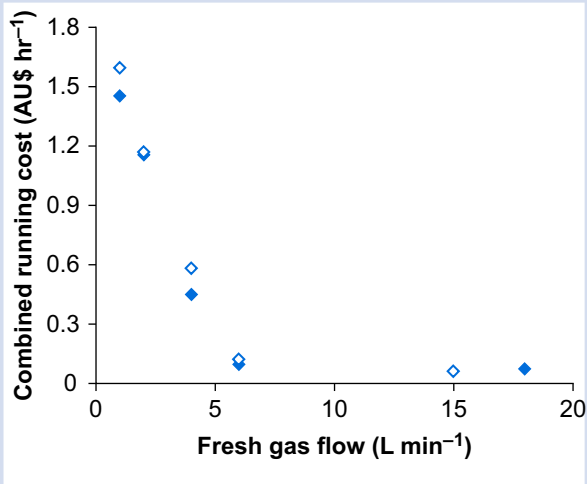


Fig 3. Hourly combined running cost (absorbent canister and medical gases) at various fresh gas flows for DG (◆) and GE (◇) anaesthetic machines. DG, Dräger Primus; GE, GE Aisys CS²

expiratory phase or adding an inspiratory pause (i.e. decreasing the I:E ratio) can both lead to greater CO₂ elimination from the circle, thus prolonging time to CO₂ absorbent exhaustion. Further studies are needed to explore the interplay between FGF, ventilatory parameters, and CO₂ production and elimination for modern ventilators.

Despite differences in the details of their circuit designs, the results from the two anaesthetic machines tested in this study were similar. However, it cannot be assumed that our results can be generalised to other circle systems. For example, some modern anaesthesia machines incorporate a turbine that circulates gas throughout the entire respiratory cycle. The altered mixing of gases in these circuits could

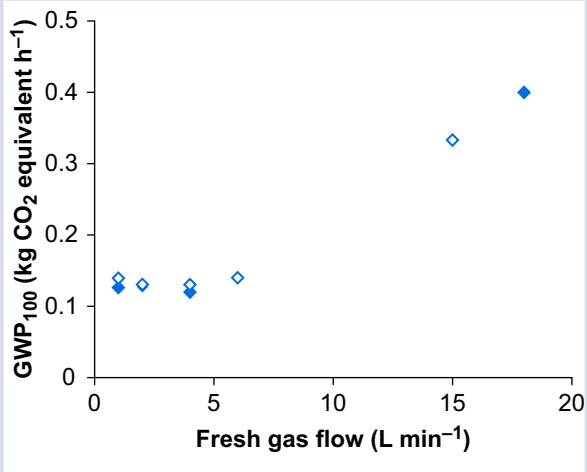


Fig 4. Environmental impact, measured as 100 yr global-warming potential, associated with various fresh gas flows for DG (◆) and GE (◇) anaesthetic machines. DG, Dräger Primus; GE, GE Aisys CS²

change the relationship between FGF and time to CO₂ absorbent exhaustion.⁵

The absorbent canisters in this study were subjected to continuous ventilation until exhaustion, whereas usage patterns during clinical practice usually include pauses between cases. We are not aware of any studies examining the effects of intermittent pauses in gas flow on absorbent consumption.

Our test lung differed from human subjects in that it was not humidified and has no O₂ uptake. It is possible that moisture from the patient's expired gas may increase the humidity within the canister, thereby influencing its CO₂ absorption efficiency. However, modern HME filters are efficient at trapping moisture from the patient, and the potential impact on circuit humidity is unlikely to be significant. Furthermore, the flow augmentation effects of O₂ uptake *in vivo* are also likely negligible.

During the longer runs at 6 L min⁻¹, ETco₂ drifted higher and over a wider range compared with lower FGFs. This wider range was attributed to fluctuations within the ball rotameter and was possibly related to fluctuations in ambient temperature. However, higher ETco₂ will result in an underestimate of the time to exhaustion, which further supports our conclusion about the effectiveness of high FGFs. Future experiments could use mass flow controllers to deliver precise CO₂ inflow.

Economic analysis was derived using local costs and may not apply to other parts of the world. However, cost data from the UK, USA, and Germany showed that our economic analysis appeared robust and potentially generalisable to other tertiary hospitals worldwide that use piped gas supplies. Although the fractional cost saving derived from the use of high FGFs is significant, the absolute cost saving is small and represents less than 4% of the total anaesthetic cost (excluding personnel).¹¹ However, a change in practice to using higher FGFs could nonetheless be important as it is simple to implement, associated with no significant drawbacks, and the cost saving could be significant when considered on a worldwide scale.

Within the aforementioned limitations, we have shown that a significant cost saving may be derived from increasing FGF to reduce CO₂ absorbent consumption, with minimal adverse impact to the environment. We suggest that 'high-flow anaesthesia', with FGF around 6 L min⁻¹, is a viable cost-saving strategy when using a circle system for anaesthetic maintenance without inhalational anaesthetic agents in adults.

Authors' contributions

Study design: GZ, AA, TM, SK
 Data collection: GZ, JJ, SK
 Data analysis: GZ, AA, TM, JJ
 Writing of first draft: GZ
 Revision of paper: all authors

Declarations of interest

The authors declare that they have no conflicts of interest.

Funding

Sydney Local Health District.

Acknowledgements

The authors thank L. Nguyen and C. Wang from the Department of Biomedical Engineering, and K. Duncan and R. Traill from the Department of Anaesthesia at Royal Prince Alfred Hospital for their kind assistance with equipment set-up.

Appendix A. Supplementary data

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.bja.2020.07.043>.

References

- Poopalalingam R, Goh MH, Chan YW. The effect of heat and moisture exchanger and gas flow on humidity and temperature in a circle anaesthetic system. *Singapore Med J* 2002; **43**: 563–5
- Nunn G. Low-flow anaesthesia. *Contin Educ Anaesth Crit Care Pain* 2008; **8**: 1–4
- Weisser D. A guide to life-cycle greenhouse gas (GHG) emissions from electric supply technologies. *Energy* 2007; **32**: 1543–59
- International Organization for Standardization. *Environmental management—life cycle assessment—principles and framework*. Available from, <https://www.iso.org/standard/37456.html>. [Accessed 27 June 2020]
- Hendrickx JFA, De Ridder SPAJ, De Houwer A, et al. In vitro performance of prefilled CO₂ absorbers with the Aisys®. *J Clin Monit Comput* 2016; **30**: 193–202
- Omer M, Hendrickx JFA, De Ridder S, et al. In vitro performance of prefilled CO₂ absorbers with the Zeus®. *J Clin Monit Comput* 2018; **32**: 799–806
- Hinz J, Rieske N, Schwien B, et al. Cost analysis of two anaesthetic machines: “Primus®” and “Zeus®”. *BMC Res Notes* 2012; **5**: 3
- Ohrn M, Gravenstein N, Good ML. Duration of carbon dioxide absorption by soda lime at low rates of fresh gas flow. *J Clin Anesth* 1991; **3**: 104–7
- Wilkes AR. Heat and moisture exchangers and breathing system filters: their use in anaesthesia and intensive care. Part 1—history, principles and efficiency. *Anaesthesia* 2011; **66**: 31–9
- Braz JRC, Braz MG, Hayashi Y, et al. Effects of different fresh gas flows with or without a heat and moisture exchanger on inhaled gas humidity in adults undergoing general anaesthesia. A systematic review and meta-analysis of randomised controlled trials. *Eur J Anaesthesiol* 2017; **34**: 515–25
- Johansson A, Lundberg D, Luttröpp HH. The effect of heat and moisture exchanger on humidity and body temperature in a low-flow anaesthesia system. *Acta Anaesthesiol Scand* 2003; **47**: 564–8
- Henriksson BA, Sundling J, Hellman A. The effect of a heat and moisture exchange on humidity in a low-flow anaesthesia system. *Anaesthesia* 1997; **52**: 144–9
- Struys MMRF, Bouche MPLA, Rolly G, et al. Production of compound A and carbon monoxide in circle systems: an in vitro comparison of two carbon dioxide absorbents. *Anaesthesia* 2004; **59**: 584–9

Handling editor: Hugh C Hemmings Jr